



Whitehall Manufacturing[®]
 Manufacturer of Healthcare and Rehabilitation Products since 1946

Dignity Suite[™] Healthcare and Ligature Resistant Products

Division of Acorn Engineering Company[®]



A MEMBER OF



Whitehall Ligature Resistant ADA Compliant Bariatric Corterra[®] Basin

Model WHD-BSN



Patent US D961740 S

WHD-BSN-WH3375-SO

Fixture May Show Some Available Options

The BestCare[®] Dignity Suite[™] is a curated collection of ligature-resistant bathroom fixtures and accessories. Designed to create a peaceful and well-balanced environment, the Dignity Suite[™] is stylish and sleek while simultaneously protecting patients' safety.

Dignity Suite[™] Ligature Resistant Corterra[®] Basin is engineered to combine the look and feel of commercial grade designer Basins with durability and economy in mind. Each standard height Washbasin complies with ADA, ANSI, and UFAS requirements. Compliance is subject to the interpretation and requirements of the local code authority.

Basin is constructed of Corterra[®] Solid Surface Polymer Resin, is Greenguard Gold listed and conforms with ANSI Z124.3 and ANSI Z124.6 and is ANSI/ICPA SS-1 compliant. Color furnished is Blanco Gloss OCC11 (White). Unit includes ligature resistant grid strainer with waste piping and 1-1/2" Brass P-Trap. Standard Deck includes Faucet drilling with 3 Holes on 4" Centerset. Unit is also available with 3 Holes on 8" Centerset.

Optional Ligature Resistant Faucets are available (WH3375-SO shown). See **Individual BestCare Specification Sheets for 4" & 8" Centerset Faucet selections.**

Optional Mounting Carrier (-MC) available for Bariatric applications to provide fixture rated at 750 lbs. Note: Appropriate Wall depth required for Carrier.

Optional Mixing Valve (WHST70-12) delivers tempered water flow by compensating for pressure and temperature fluctuations and is ASSE 1070 compliant. Valve is factory set to 105° Fahrenheit. Operating range is 30 PSI to 100 PSI.

Enclosure conceals P-Trap and optional valve assembly and is constructed of heavy gage, type 304 stainless steel. Enclosure assembly is Enviro-glaze[®] Matte White EG-26 powder coat finish. Vandal resistant fasteners are provided to facilitate installation.

GUIDE SPECIFICATION

Provide Whitehall Ligature Resistant Corterra[®] Washbasin. Unit with 34" standard rim height to conform with ANSI, UFAS and ADA Accessibility Standards. Basin, Backsplash and Side Splashes to be constructed of Corterra[®] Solid Surface Polymer Resin and shall be Greenguard Gold listed. Basin shall include Ligature Resistant Side Splashes, Ligature Resistant Grid Strainer, Waste Piping and 1-1/2" P-Trap. Provide drilling for (Specify Whitehall Bestcare[®] model) Faucet. Washbasin shall conform to ANSI Z124.3 and ANSI Z124.6. P-Trap Enclosure to be constructed of heavy gage, type 304 stainless steel and powder coated white.

Please visit www.whitehallmfg.com for most current specifications.



Recyclable Product



Federal Public Law 111-380 (No Lead)



Whitehall Mfg. • P.O. Box 3527 • City of Industry, CA 91744 • (800) 782-7706 • (626) 968-6681

WHD-BSN

Revised: 06/05/2025



MODEL NUMBER AND OPTIONS SELECTION:

BASE MODEL NUMBER

- WHD-BSN Ligature Resistant Corterra® Dignity Basin - 3 Hole, 4" Centerset Deck Openings
- WHD-BSN-H38 Ligature Resistant Corterra® Dignity Basin - 3 Hole, 8" Centerset Deck Openings


FAUCET SELECTION

See Individual BestCare® Specification Sheets for 4" and 8" Centerset Faucets.



(Refer to <https://www.whitehallmfg.com/faucets>)

PRODUCT OPTIONS

- MC Mounting Carrier (Rated at 750 lbs for Bariatric)
- WHST70-12 Tempering Valve With Integral Mounting Feet Brass Body With 1/2" NPT Connections
- OCC Optional Corterra® Color - Specify _____ (Blanco Gloss OCC11 Provided Standard)
 (Refer to <https://www.whitehallmfg.com/corterra-solid-surface> for available colors)

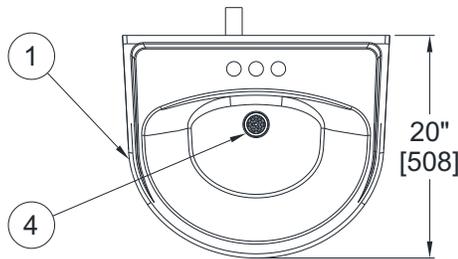

- NOTES:**
1. Dignity Basin Assembly
 2. Basin Trap Enclosure Assembly
 3. 1-1/2" OD P-Trap Waste Outlet
 4. Ligature Resistant Strainer

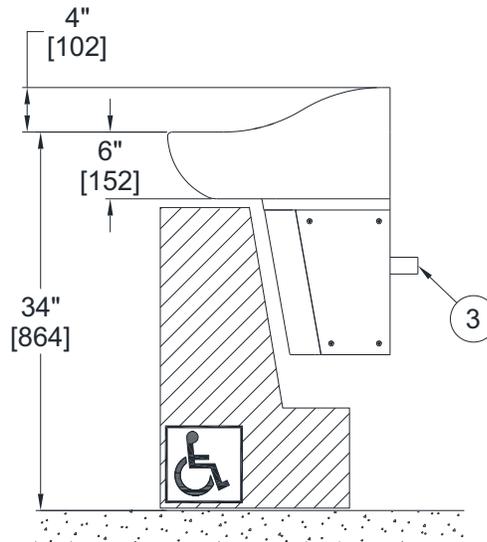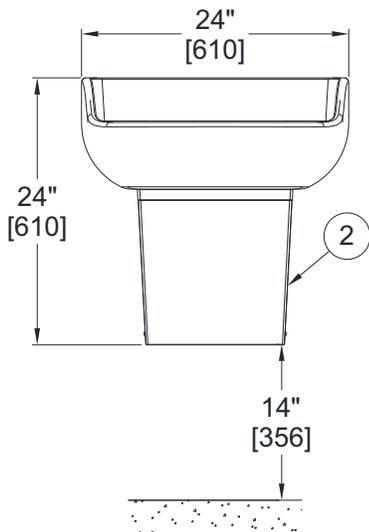

WHD-BSN

DISCLAIMER:

This product is designed to decrease the probability that it may be utilized as an apparatus for ligature. It is not a replacement for professionals who are trained in the proper evaluation, management and supervision of persons at risk of suicide.

⚠ WARNING: Cancer and Reproductive Harm - www.P65Warnings.ca.gov

SELECTION SUMMARY & APPROVAL FOR MANUFACTURING

Model Number & Options _____ Quantity _____
 Company _____ Date _____
 Contact _____ Title _____
 Approval for Manufacturing/Signature _____

All dimensions are nominal and subject to manufacturer's change without notice. Whitehall assumes no responsibility for use of void or superseded data © Whitehall Manufacturing, Member of Morris Group International. Please visit www.whitehallmfg.com for most current specifications.